

Medical Applications of Electromagnetic Waves



Shiban Kishen Koul

Life Fellow IEEE, IETE, Fellow INAE

Indian Institute of Technology Delhi (INDIA)

s.k.koul@ieee.org





Healthcare-Future

Wealth is not Health


Health is Wealth

- **More Stressful Lifestyle**
- **Extremely Large Number of Patients**
- **Need to learn from New Medical Threats**
- **Non-invasive Diagnostic procedures Required**
- **Targeted Drug Delivery Systems Required**
- **Need for Remote/Self Medical Assistance**
- **Reduction in medical costs**

Enablers: MHz to THz Technologies, AI, ML, Cloud Computing, Smart Sensors, 3D printing Technology




What are Electromagnetic Waves?

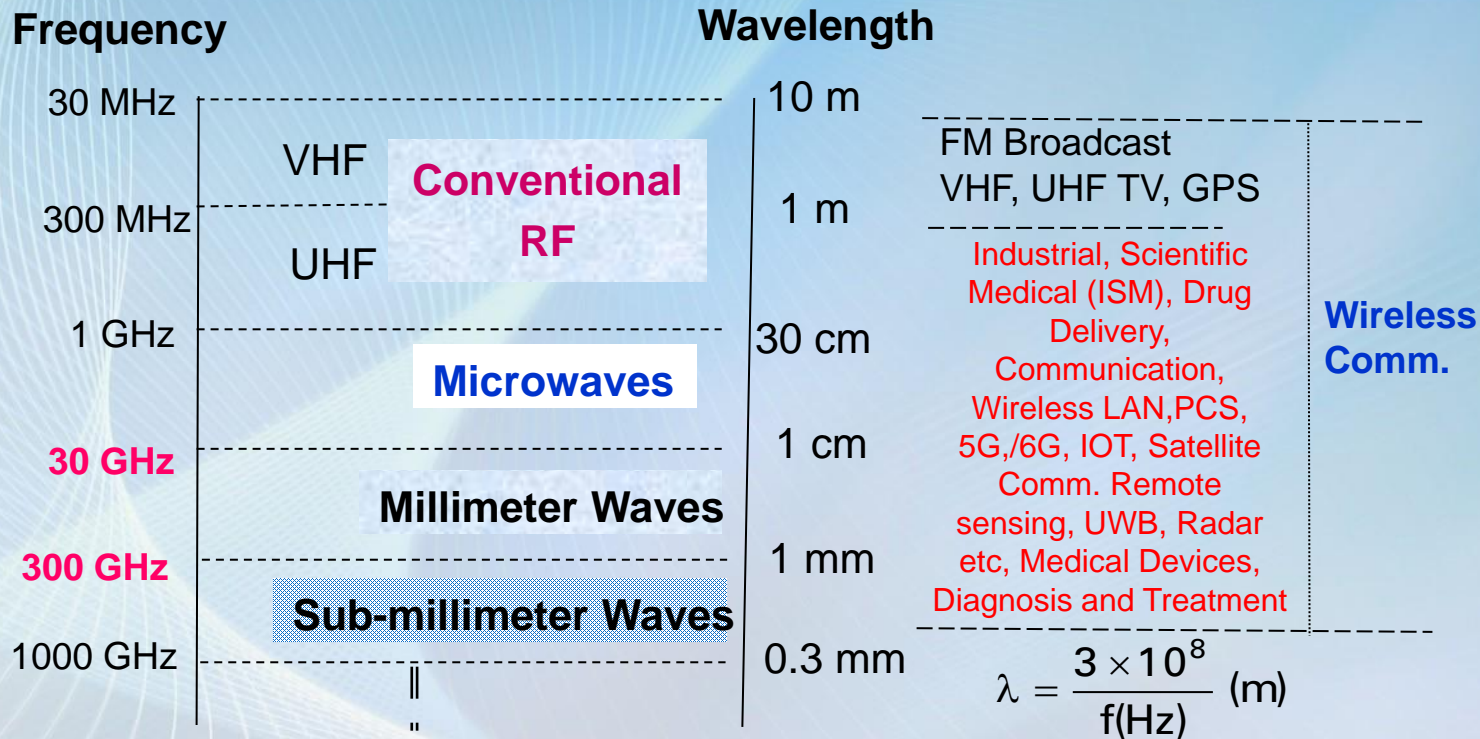

Millimeter Waves and Sub-Terahertz Occupy Frequency Spectrum from 30-300 GHz



Why Millimeter and Sub-THz Waves?


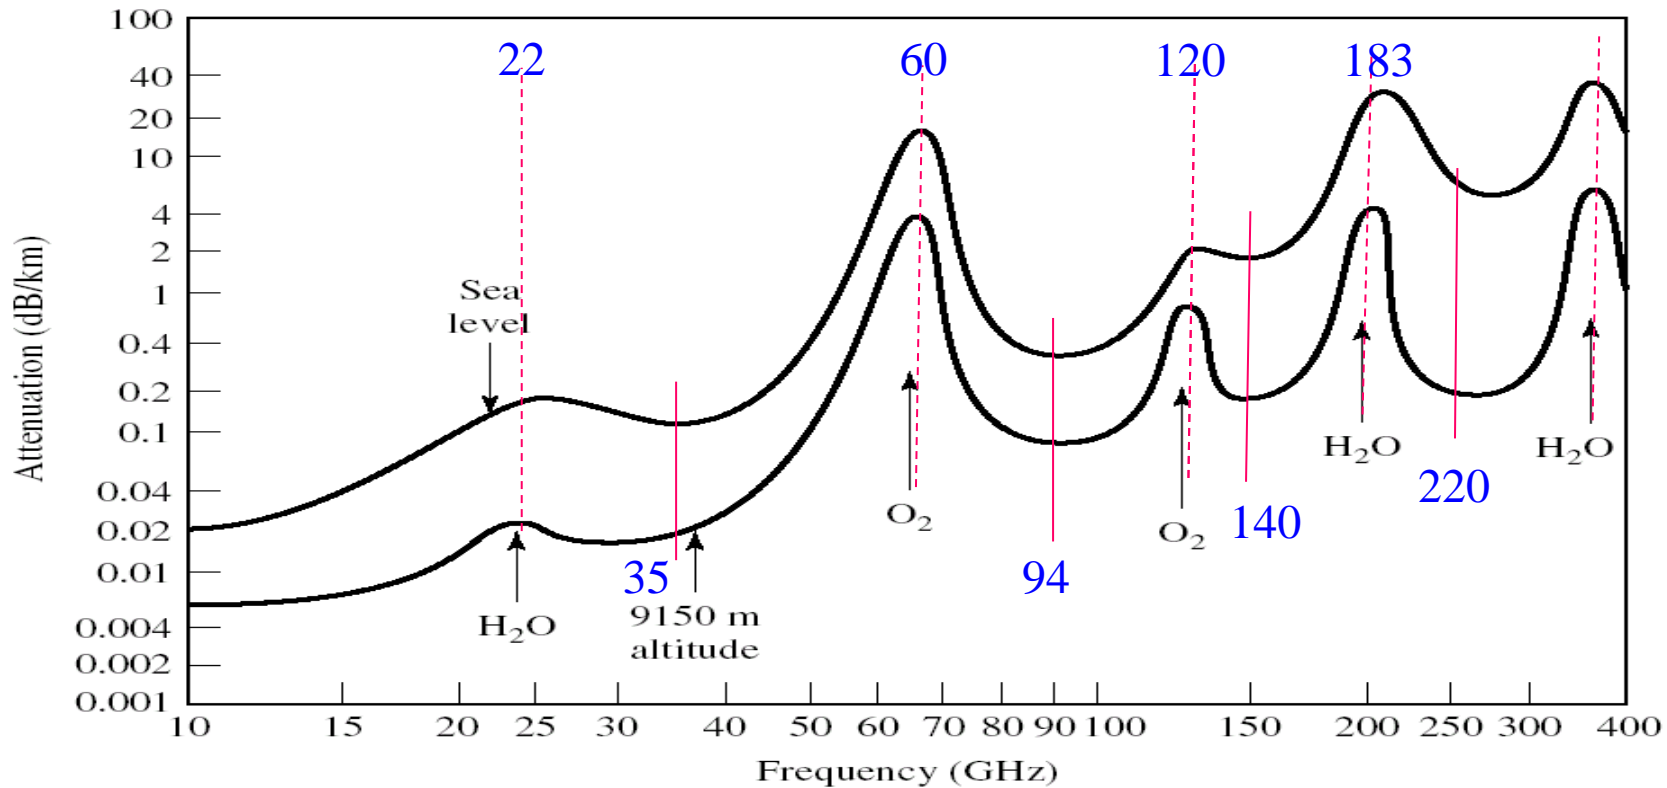




Wearable Non-invasive Sensor Based System

Uses Photodetectors at the back for O2 sensing, Crown to monitor heart beats (ECG) and distance covered for Cardio Fitness


Uses RF Links to Transmit Data to Mobile devices

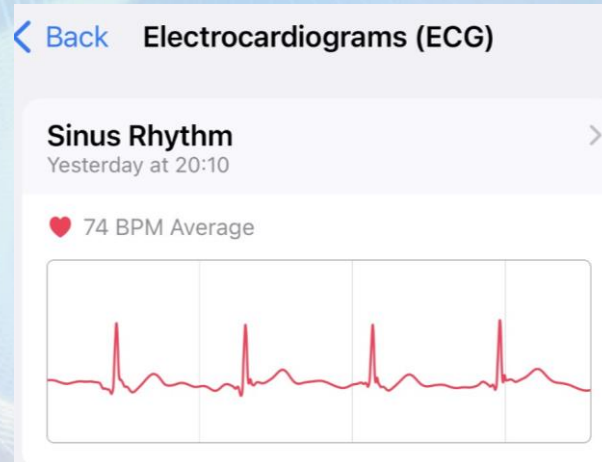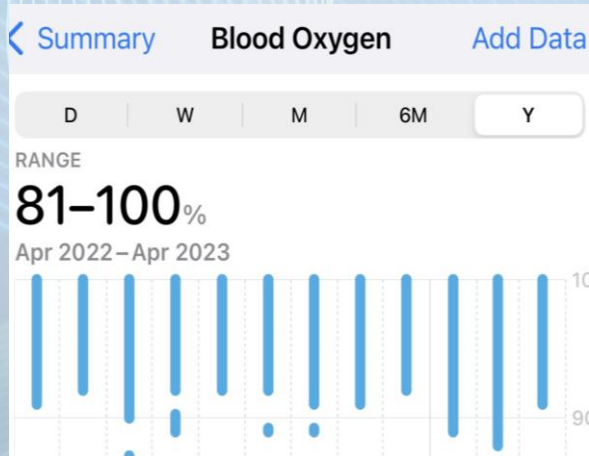


Wearable Sensor based Continuous Glucose Monitor



Millimeter Wave Non-Invasive Glucose Monitoring

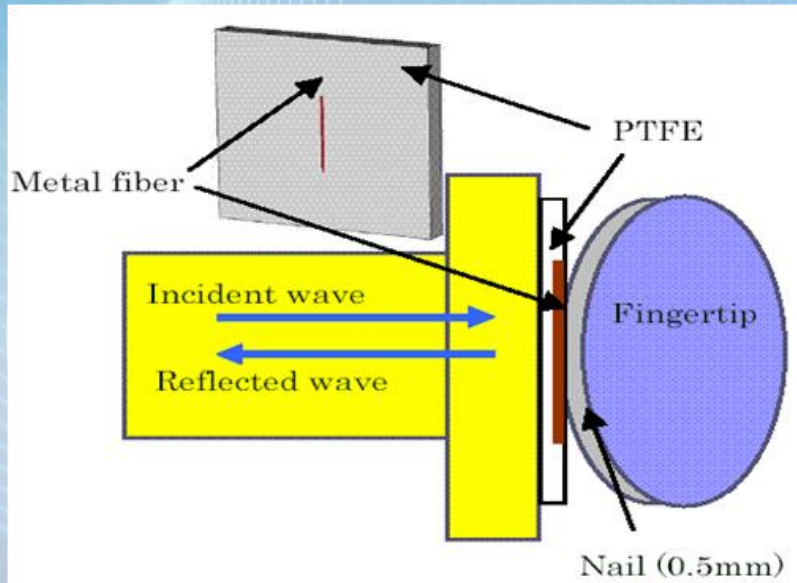

60 GHz cavity system to measure blood sugar

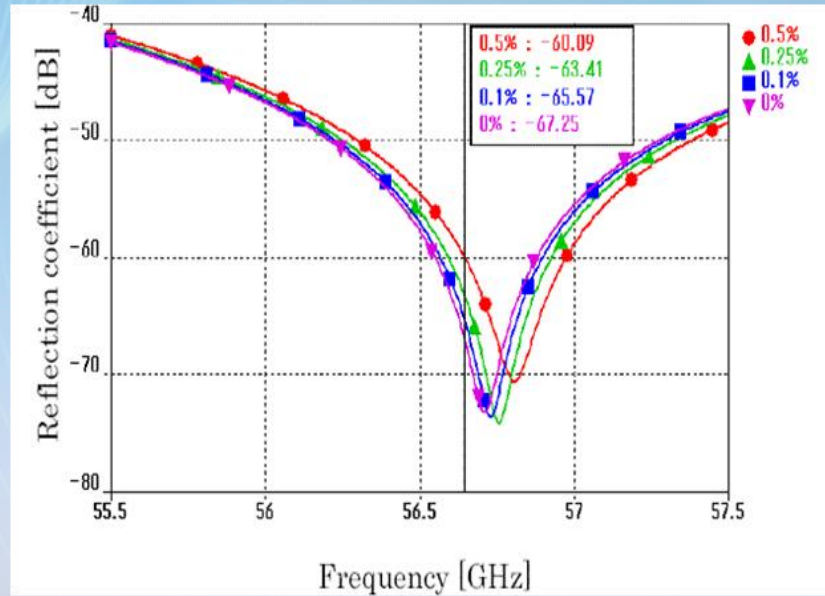

Cavity resonant frequency changes depending on the blood glucose level

Device has huge Potential for Commercialization

Source: Yoshio Nikawa, APMC 2007



Sub-THz Sensor Developmental

Development of
Dielectric
characterization
Method



- Designing and testing of liquid and semi-solid material dielectric characterization method in the selected frequency regime.

Development and
characterization
of Tissue
Mimicking Models

- Development of phantoms resembling electrical properties of Skin with blood vessels in the selected frequency regime.




Data acquisition and
Output Results
setup

LIQUID DIELECTRIC CHARACTERIZATION ABOVE 100 GHz

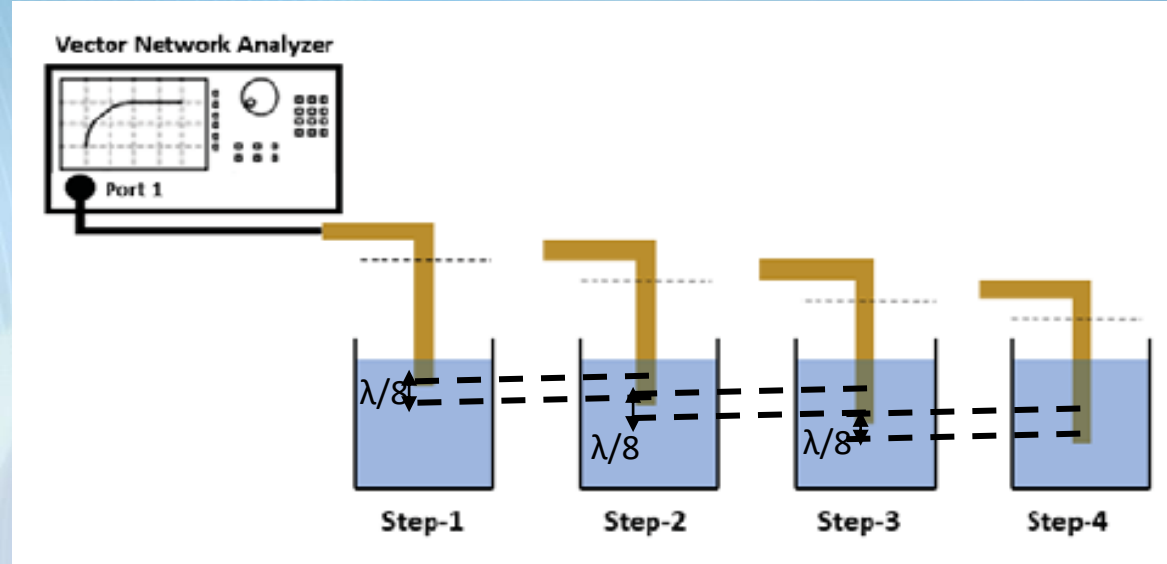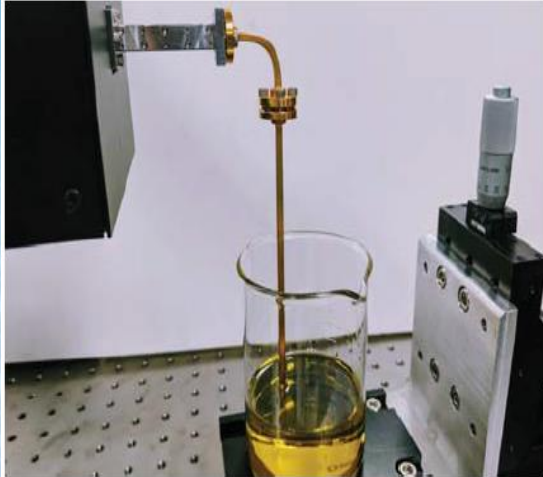

Source: S. Sahin, N. K. Nahar and K. Sertel, "Waveguide Probe Calibration Method for Permittivity and Loss Characterization of Viscous Materials," *2020 94th ARFTG Microwave Measurement Symposium (ARFTG)*, San Antonio, TX, USA, 2020, pp. 1-3, doi: 10.1109/ARFTG47584.2020.9071773.

DIELECTRIC CHARACTERIZATION OF VISCOUS LIQUIDS

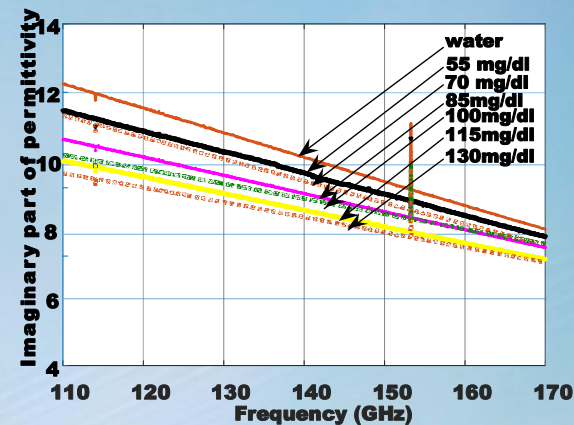
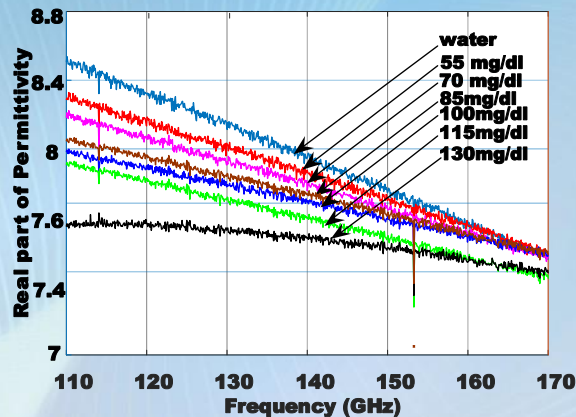
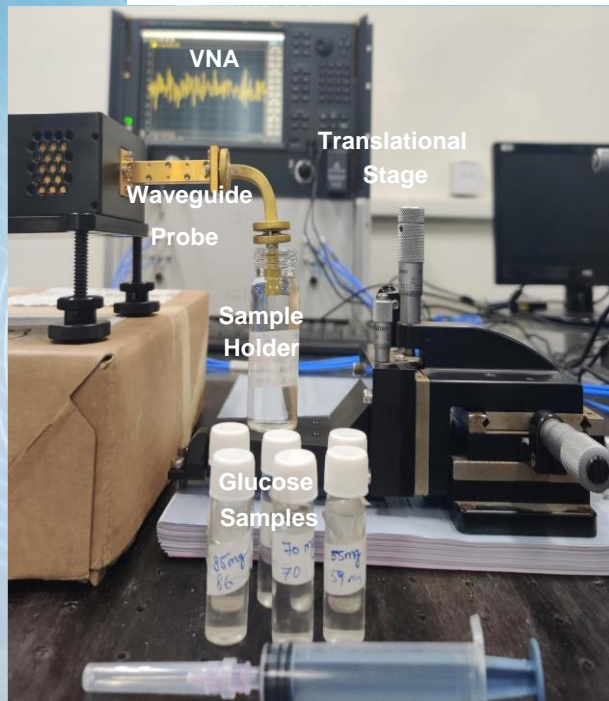


- Obtain complex dielectric constants for different glucose-water mixture concentrations.
- These glucose solutions are used for developing phantoms replicating blood glucose levels.

Source: P. Kaurav, S. K. Koul and A. Basu, "Non-Invasive Glucose Measurement Using Sub-Terahertz Sensor, Time Domain Processing, and Neural Network," in *IEEE Sensors Journal*, vol. 21, no. 18, pp. 20002-20009, 15 Sept.15, 2021.




Sub-THz Non-Invasive Glucose Monitoring

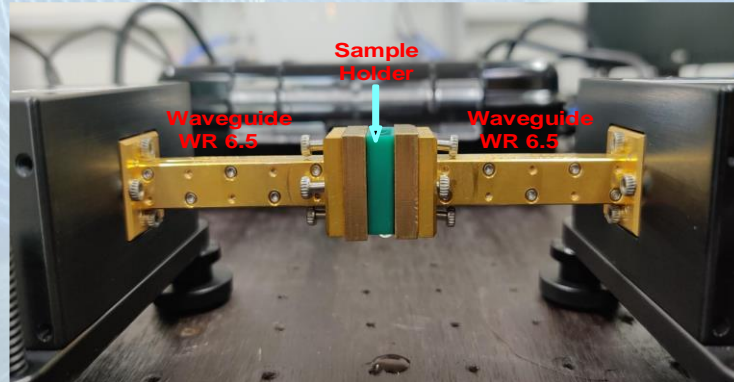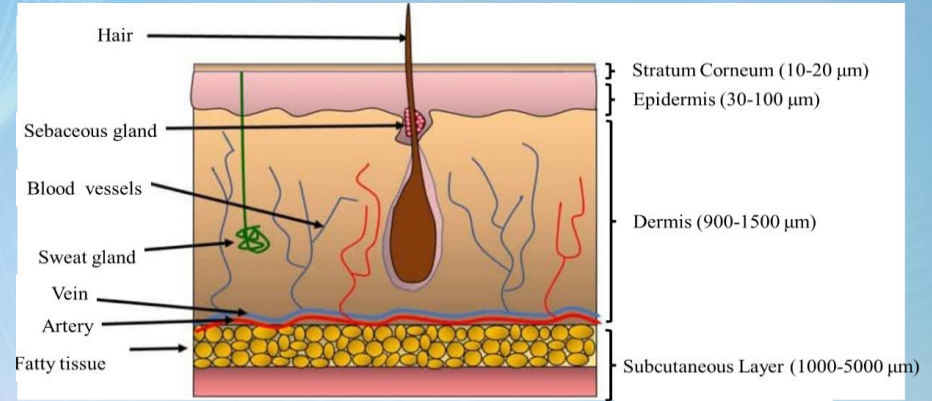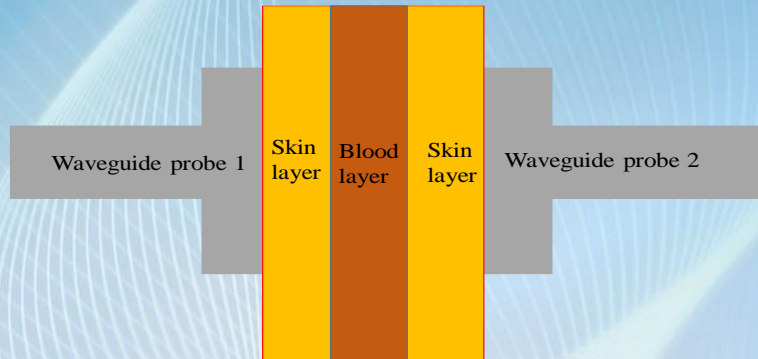

- **Electromagnetic Sensor used is WR 6.5 Waveguide Probe**
- **Phantom to mimic skin area between thumb and index finger (Thumb- index Web Space) is used in this study.**
- **Both Transmission or Reflection of sub-THz wave can be used**


Sub-THz Non-Invasive Glucose Monitoring

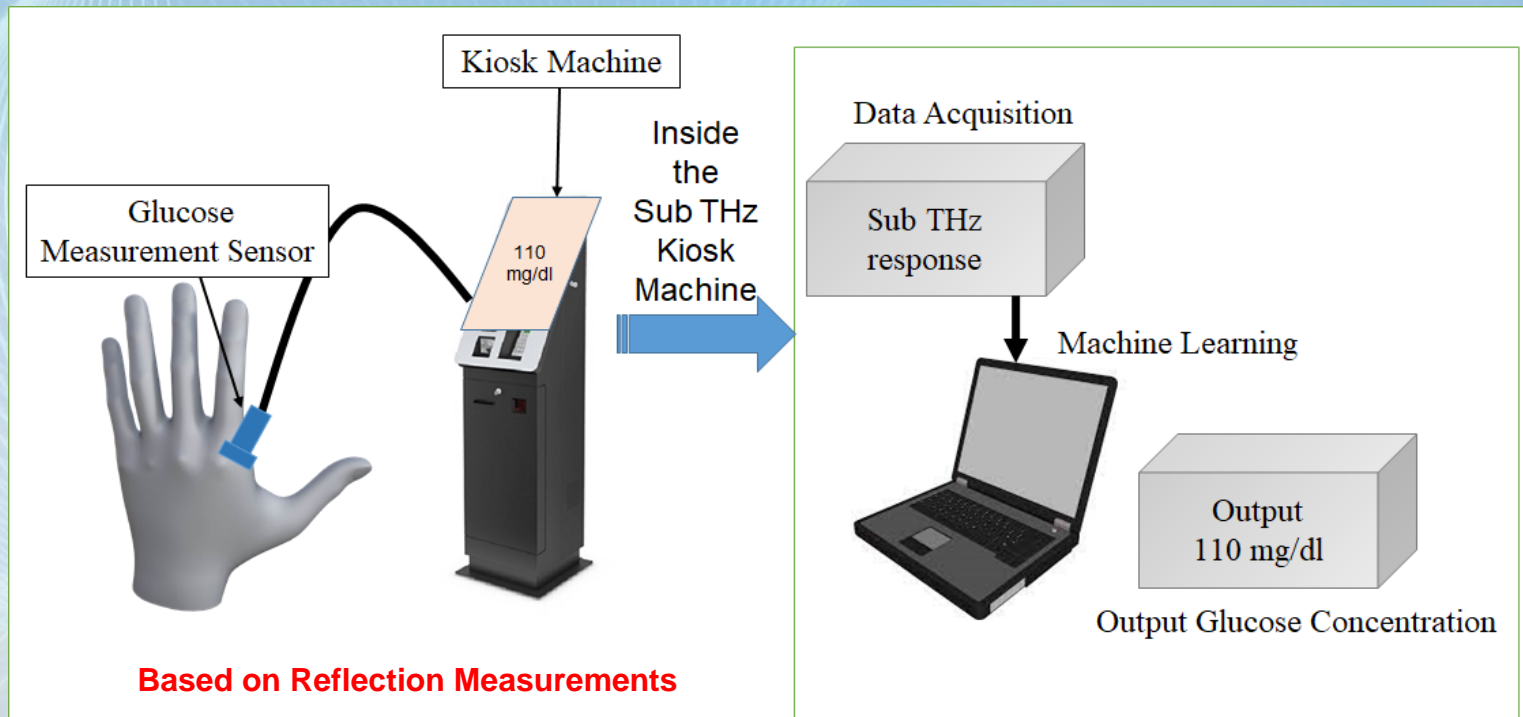



Source: P. Kaurav, Shiban K Koul and Ananjan Basu, IEEE Sensor Journal, Sept 2021

Sub-THz Non-Invasive Glucose Monitoring

1. Sub THz Waveguide Sensors

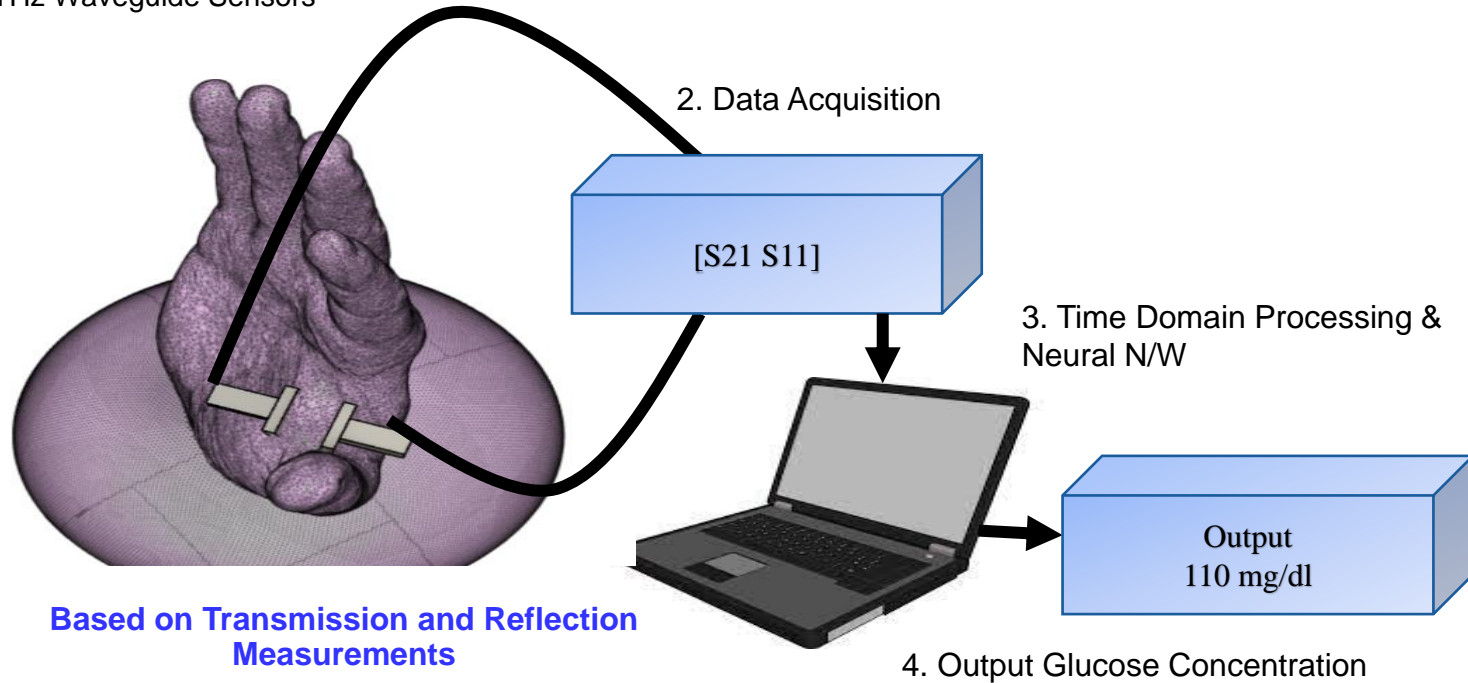


Sub-THz Non-Invasive Glucose Monitoring

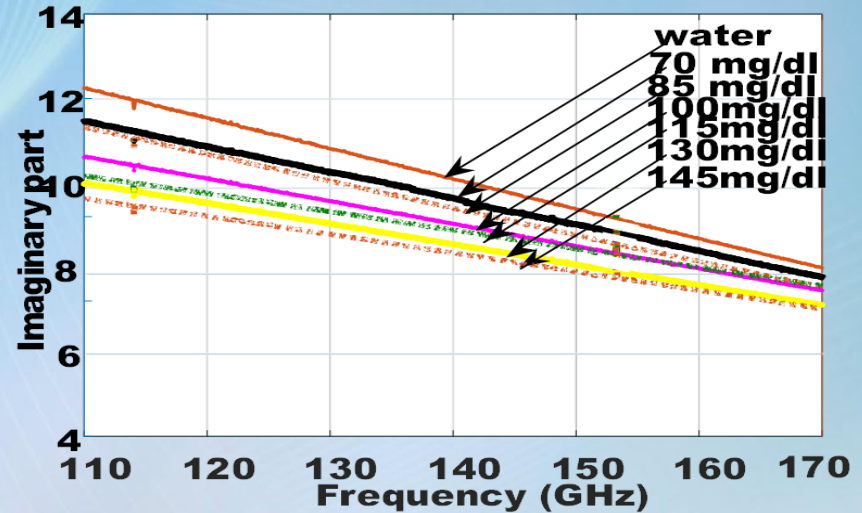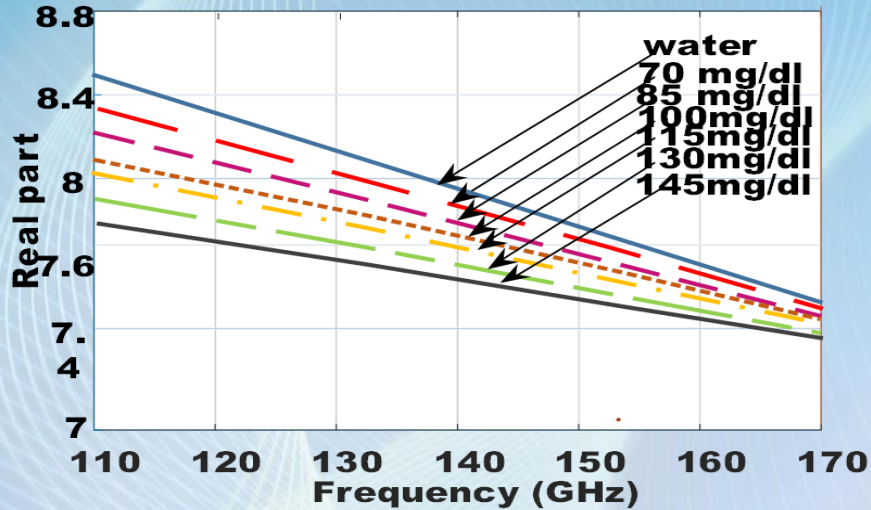

Real and Imaginary Parts of dielectric constant as a function of frequency for various concentrations of Glucose

Source: Shibani K Koul and P. Kaurav, Sub THz Sensing Technology for Biomedical Applications, Springer 2022

CONVERSION OF S-PARAMETERS TO GLUCOSE CONCENTRATION

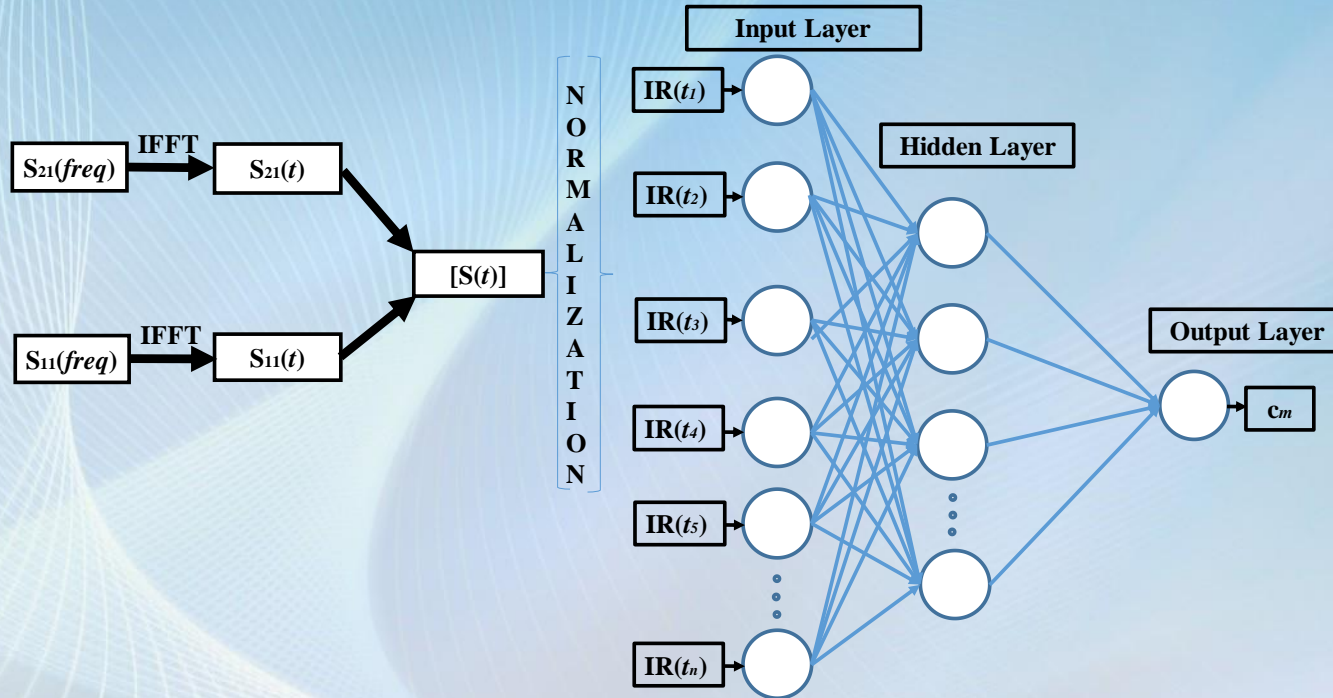

Obtaining glucose levels from S parameters using Levenberg-Marquardt algorithm based NN model



Tumor Margin Assessment Imaging Technique in Sub-THz Band

Development and characterization of Tissue Mimicking Models


- Development of phantoms resembling electrical properties of fat, fibrous and malignant breast tissues in Sub-THz band

Sub-THz probe for differentiation and depth analysis

Data acquisition and Imaging setup




Sub-THz EM Sensor Based Breast Tumor Margin Assessment

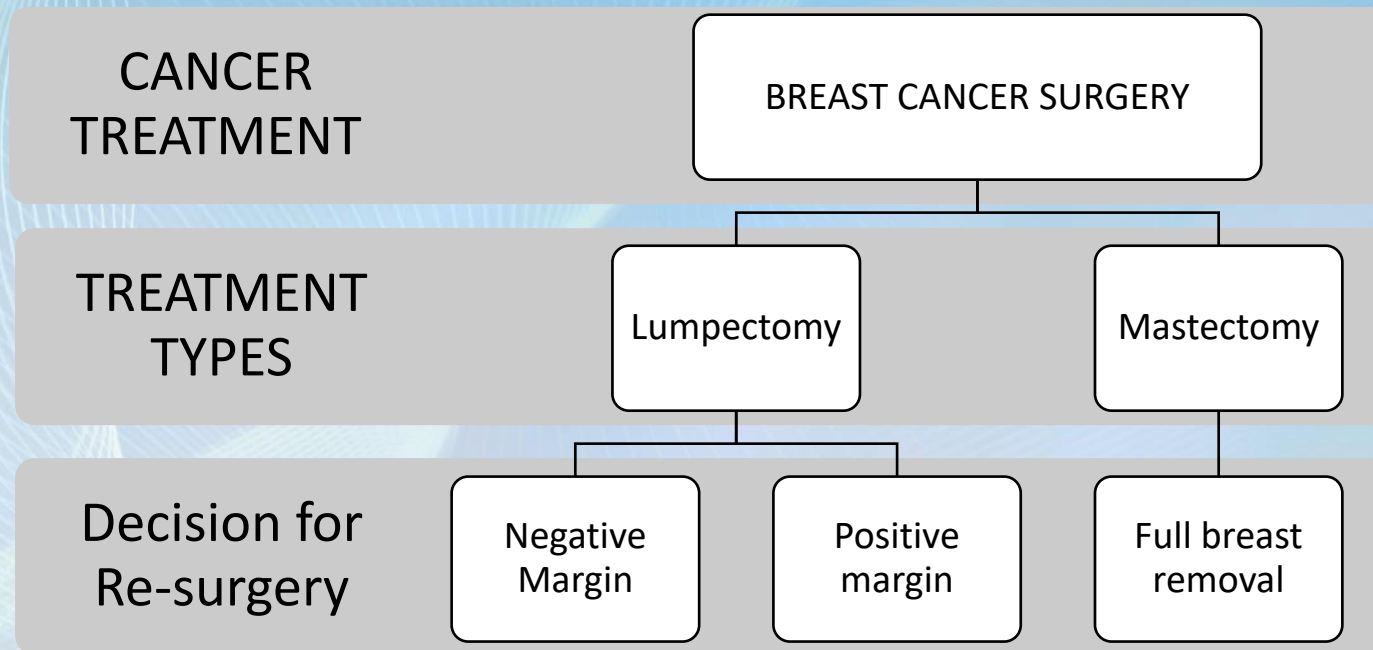

Electromagnetic Sensor: WR-65 Waveguide Probe Operating in 110-170 GHz

Sub-THz EM Sensor Based Breast Tumor Margin Assessment

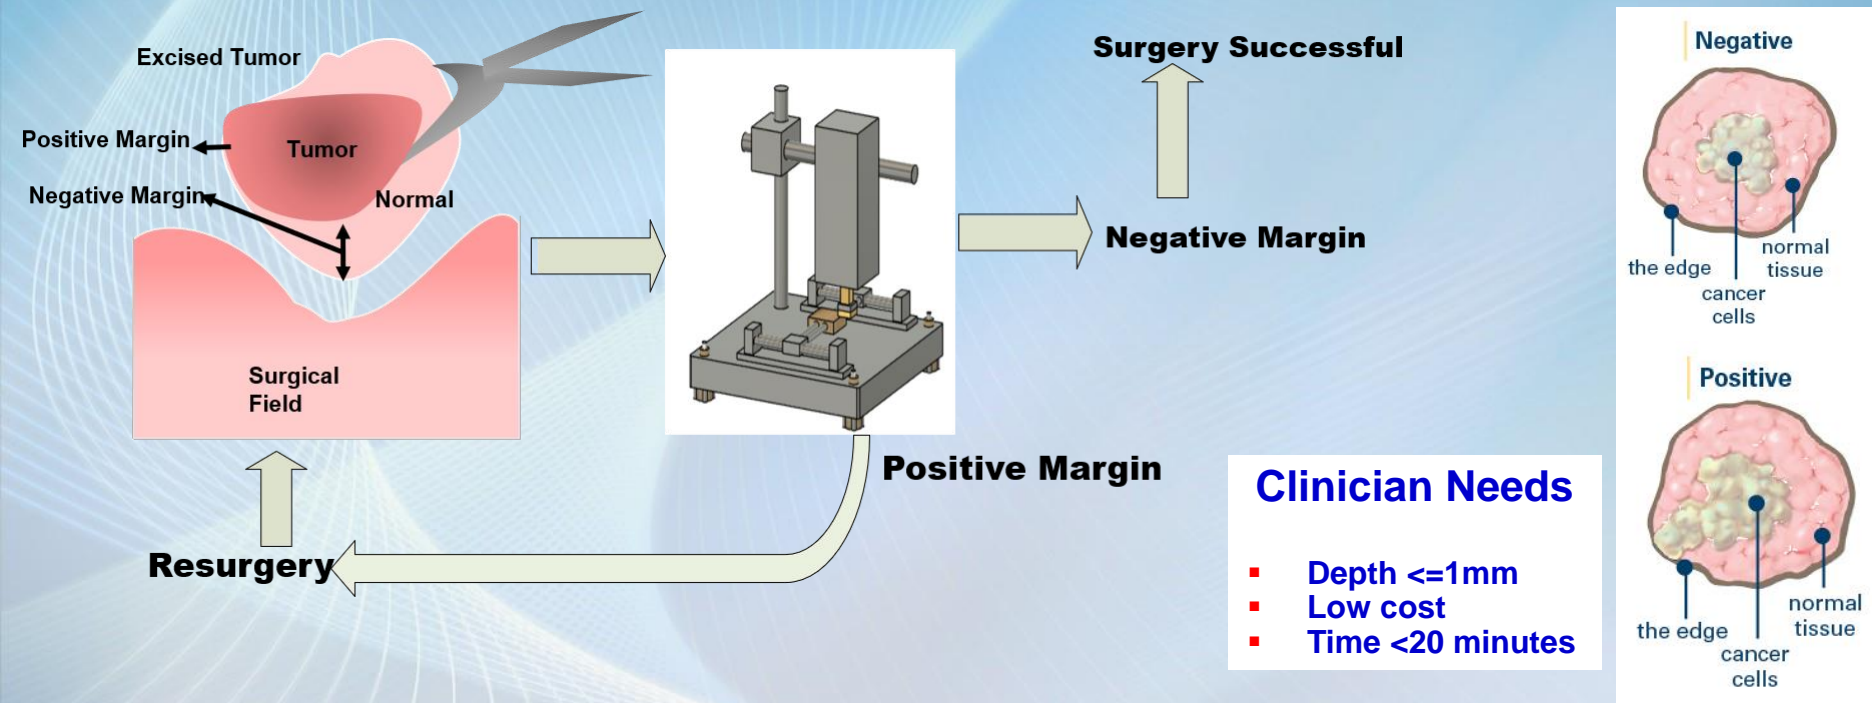

Water-Agar Based Phantoms for Mimicking Breast Tissues


- Different compositions of water-oil and agar are mixed to develop three different types of breast tissues.
- Malignant tissue: more water concentration
Fat tissue: least water concentration
- Bruggeman's effective concentration method is used to develop these tissue phantoms to mimic the dielectric properties of real tissues in the selected frequency regime (110-170 GHz)

Phantom Type	Mimicking Tissue	Composition of Phantom Constituents			
		Water (ml)	Agar (g)	Oil (ml)	Pectin (g)
Agar5%Oil20%	Malignant	70	4.6	17.5	4.2
Agar5%Oil40%	Fibrous	70	6	46.5	4.2
Agar5%Oil80%	Adipose/fat	70	18.6	280	4.2


Sub-THz EM Sensor Based Breast Tumor Margin Assessment

Requirements


- **Development of Low-Cost sub-THz Sensor**
- **Development of Breast Phantoms**
- **Manual/Automatized Measurements on Breast Phantoms**
- **Construction of images for margin assessment**

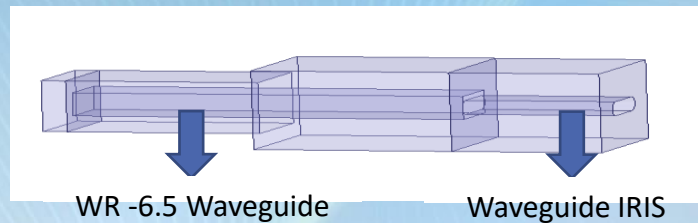


EM Sensor



**Tumor &
Healthy Breast
Tissue
Phantoms
Using
Water, Oil and
Agar**

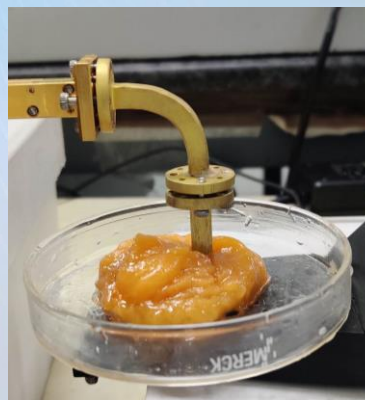

Tumor


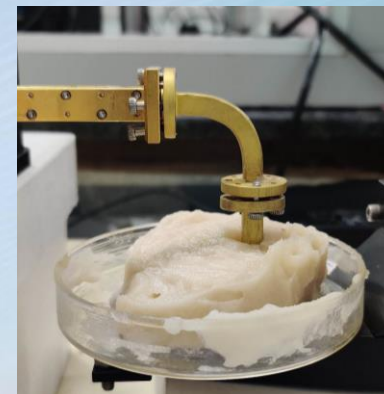


Healthy

Sub-THz EM Sensor Based Breast Tumor Margin Assessment

Imaging Setup

- Development of Low-Cost sub-THz Sensor
- Development of Breast Phantoms
- Manual/ Automatic Measurements on Breast Phantoms
- Construction of images for margin assessment

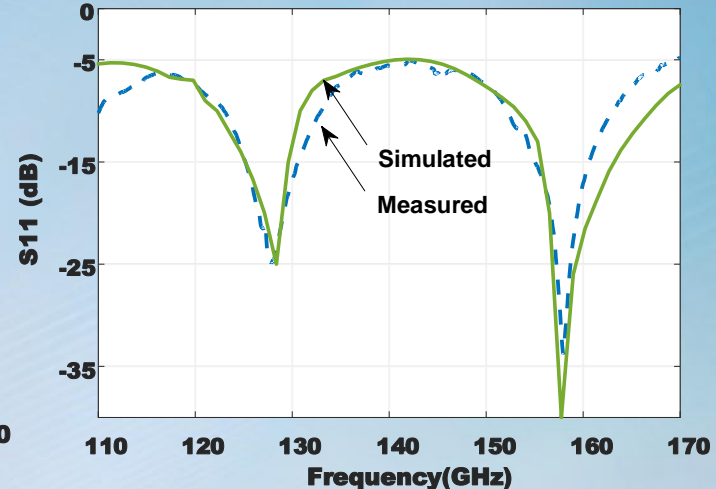
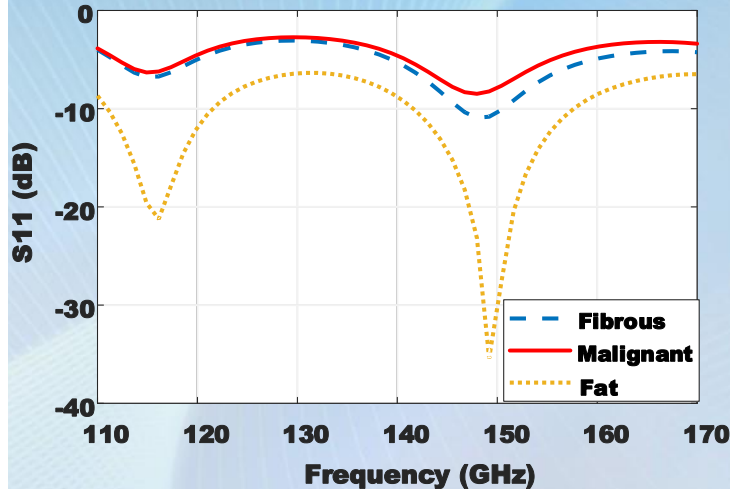


Source: P. Kaurav, Shiban K Koul and Ananjan Basu, IEEE Journal of Electromagnetics, RF and Microwave in Medicine and Biology, 2021

Sub-THz EM Sensor Based Breast Tumor Margin Assessment



Imaging Setup

- Development of Low-Cost sub-THz Sensor
- Development of Breast Phantoms
- Manual/Automatic Measurements on Breast Phantoms
- Construction of images for margin assessment

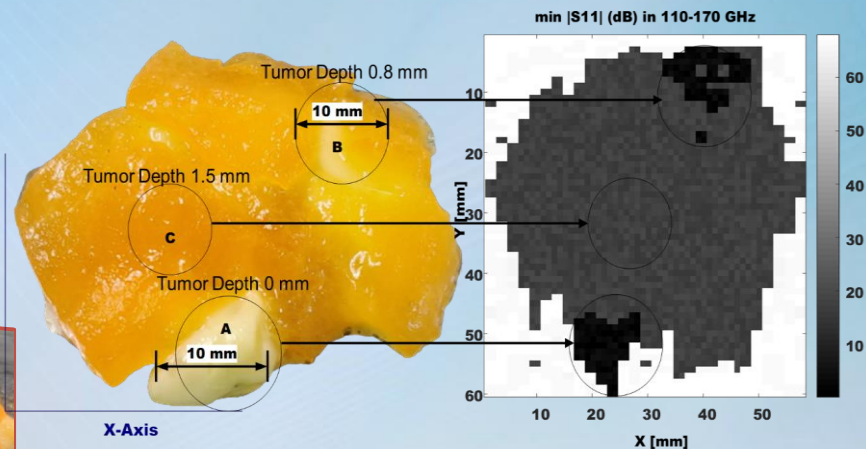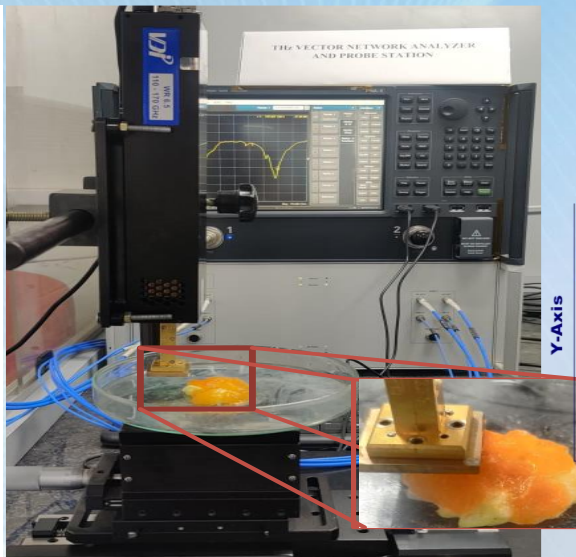


Source: Shiban K Koul and P. Kaurav, Sub THz Sensing Technology for Biomedical Applications, Springer 2022

Dental Diagnosis and Treatment

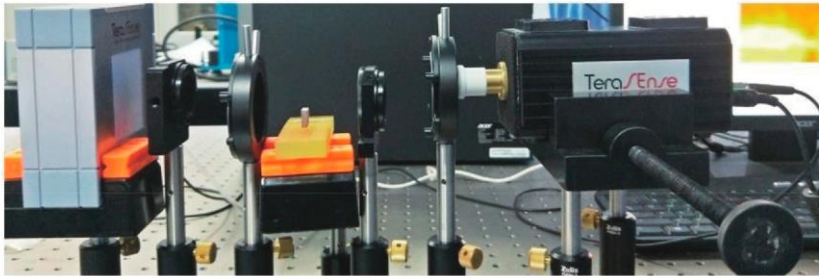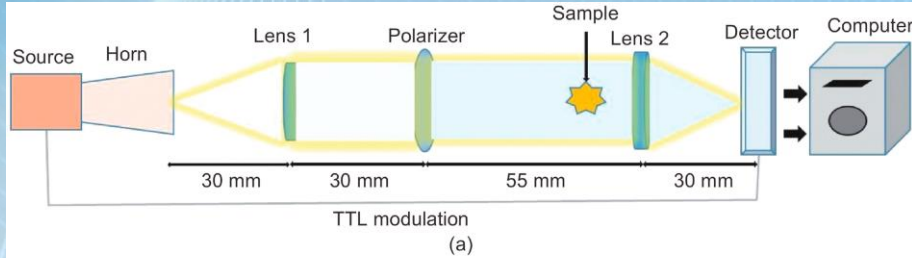

(b)

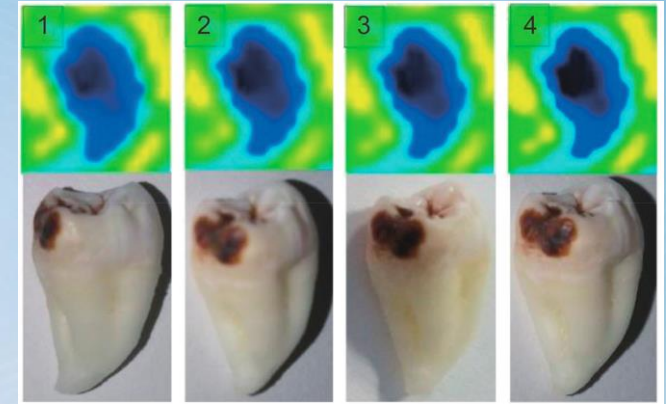

THz Imaging of Dental Caries

Dental caries are significantly lossy than a sound tooth in millimeter waves. Microwave and millimeter-wave heating for the lossy dental caries can be used as a sterilization treatment.

Source: 1. Yoshi Nikawa et al., IEEE Transactions on MTT, Nov.2000; 2. N. P.Yadav et al., Journal of Electronic Science & Technology, Sept 2021



Millimeter Wave Therapy

- All living Cells generate alternating Electromagnetic fields.
- Cell communication in our body is at 42.5, 53.6 and 61.5 GHz
- Cause of poor health is unbalance in these waves
- Communication with body cells and cell membranes requires low intensity exposure at right place using millimeter waves
- Non-Thermal Exposure using low intensity Millimeter waves is called **Millimeter Wave Therapy (MWT)**
- Research has shown healing effect for Cardiovascular disorders, diabetes, wound healing, pain relief, gastrointestinal disorders
- Reduction of toxic effects of Chemotherapy in cancer patients

MWT requires light weight affordable millimeter wave sources



Millimeter Wave Applicator


Application Scope

- Cancer
- Tumors
- Diabetes
- Prostrate
- Skin Ulcer
- Cardiovascular Diseases
- Pain Management




Radio Frequency Assisted Drug Delivery

RF Energy (EM Waves)

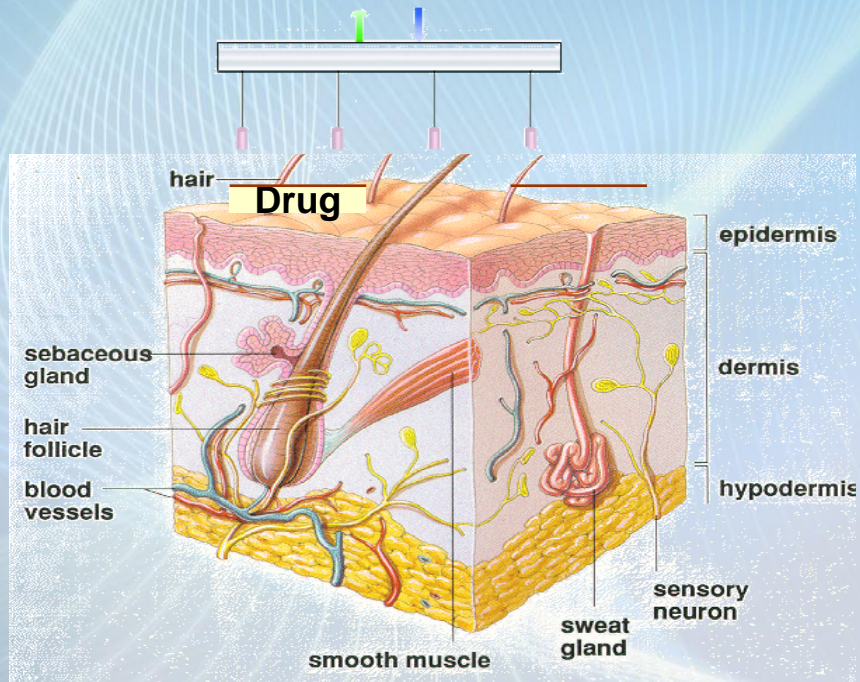


Global TDD Sales: Low Molecular Weight Drugs

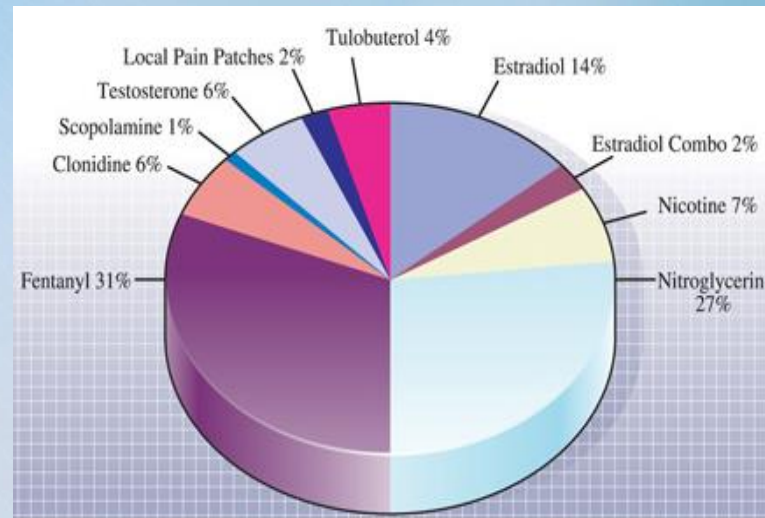

Source: PhD Thesis Rachna Prasad, CBME, IIT Delhi 1984





Radio Frequency Assisted Transdermal Drug Delivery

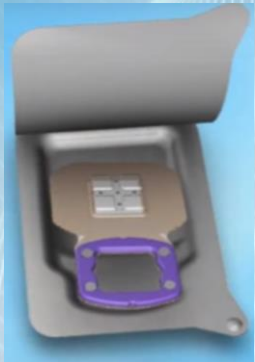

- High Molecular Weight drugs
- Hydrophilic Drugs
- Protein and peptide Drug


Microneedle Array with drug reservoir

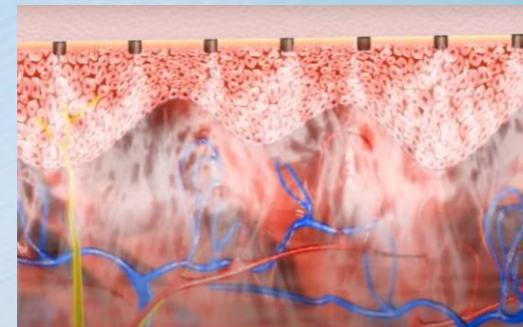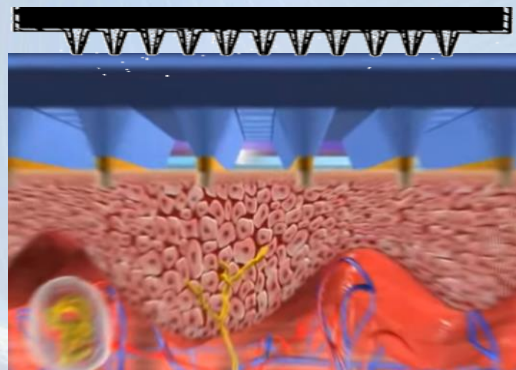

Source: Via Derm



Minimally Invasive Screening-Ingest Capsule

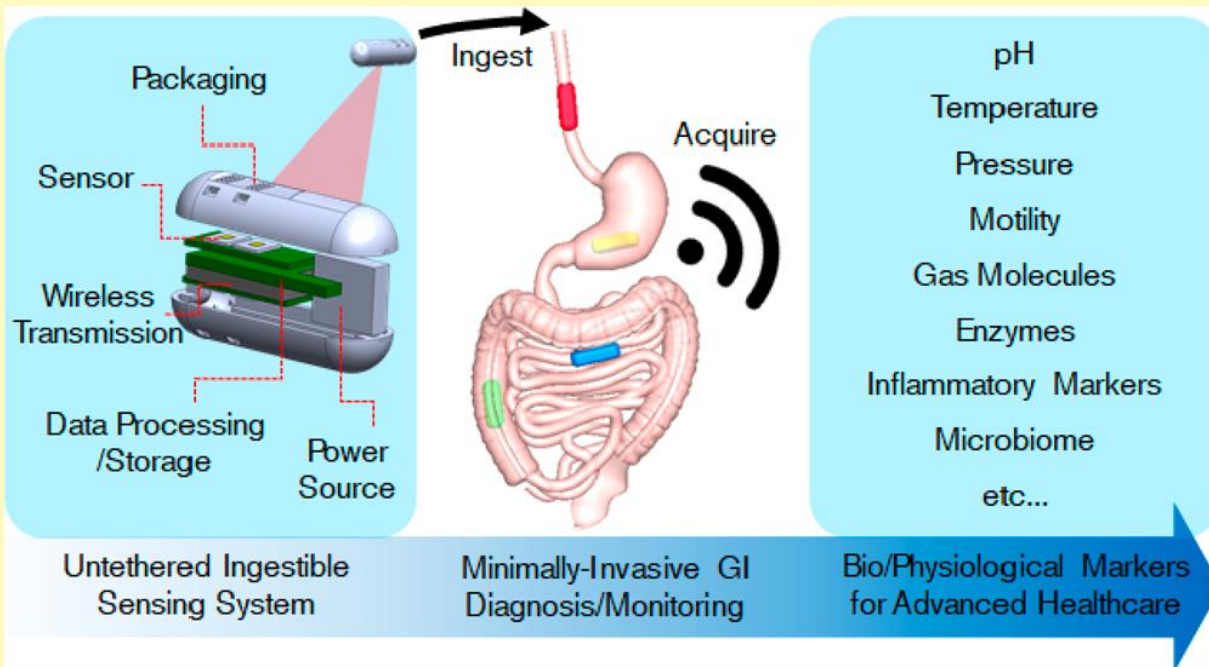

Different pill capsules are available which when digested emit EM signals that are picked by Nursing staff to ensure that the patient has taken medicine





Controlled Drug Delivery System- Endoscope Capsule


Swallowable capsule

Targeted disease
infected area

External
transmitter

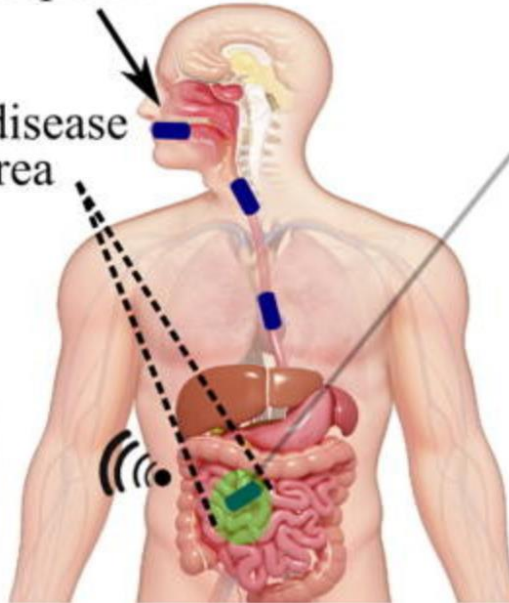

- Antenna
- Battery
- Electronic Components
- Micro reservoir
- Microneedle
- Drug

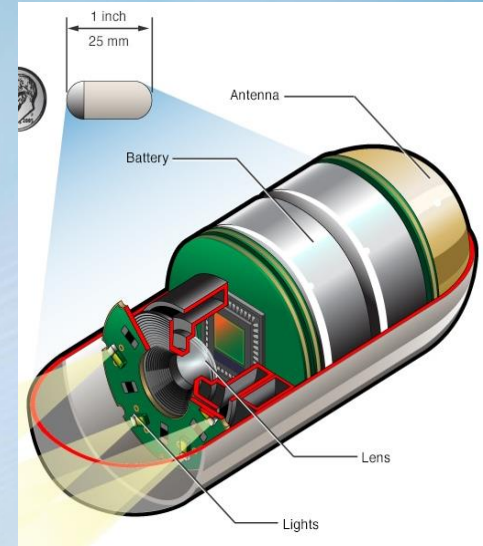




Types of Antennas for Healthcare Applications





(a)




(b)



(c)

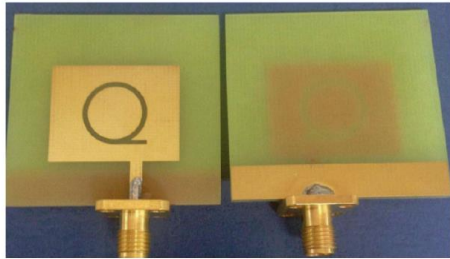


(d)

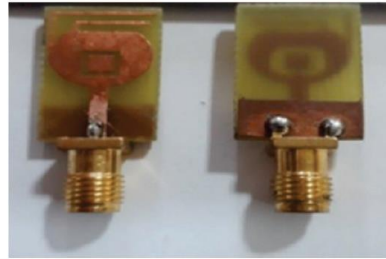


(e)

UWB Antennas

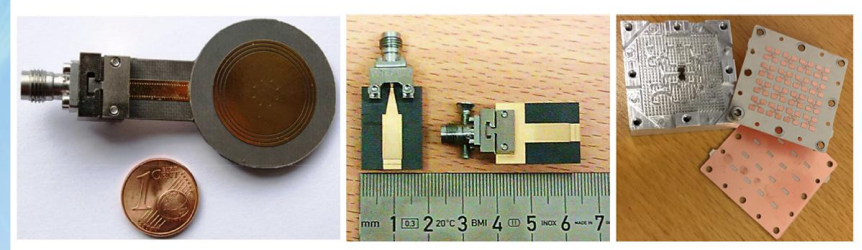

MM-wave Antennas at 60 GHz



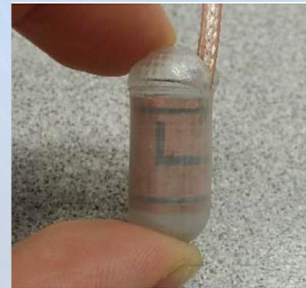


Capsule Antenna




Smart Tattoo Antenna

Flexible Antennas for Healthcare Monitoring and Rehabilitation

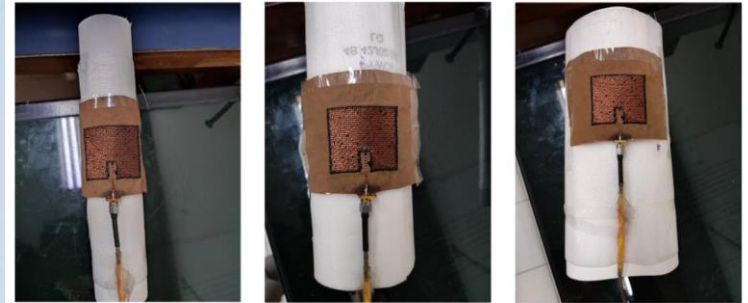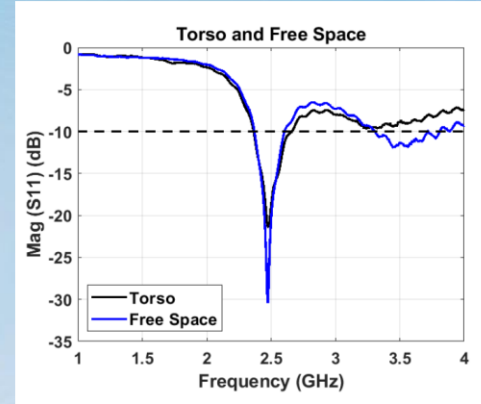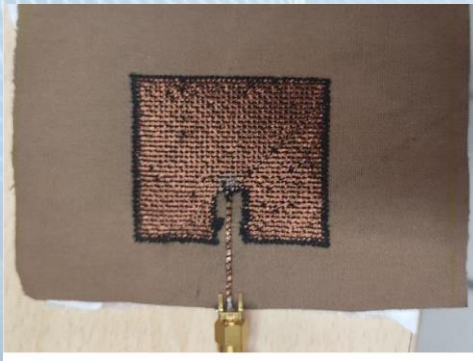


Source: Shiban Koul and Richa Bhardwaj, *Wearable Antennas and Body Centric Communication*, Springer 2021


Flexible Antennas for Healthcare Monitoring and Rehabilitation

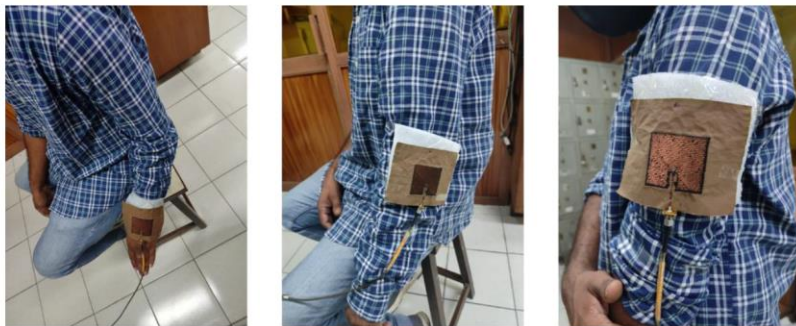

(a)

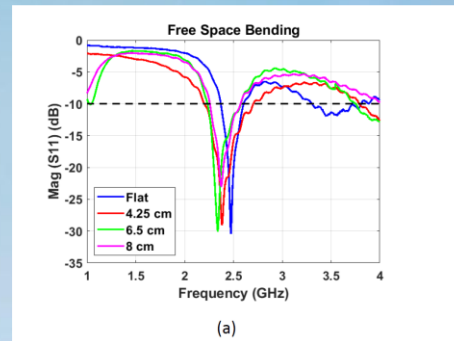


(a)

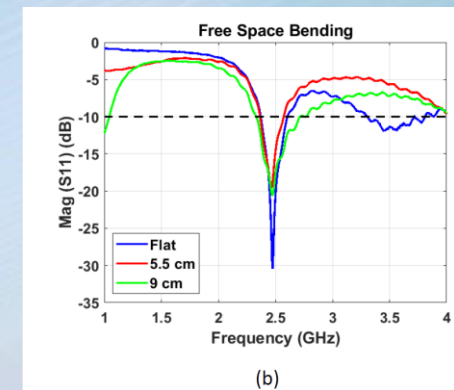

(b)

Source: Shiban Koul and Richa Bhardwaj, *Wearable Antennas and Body Centric Communication*, Springer 2021


RF Assisted Hyperthermia for Enhanced Pharmacological Effect at Lower Doses of Chemotherapy- In Vitro studies

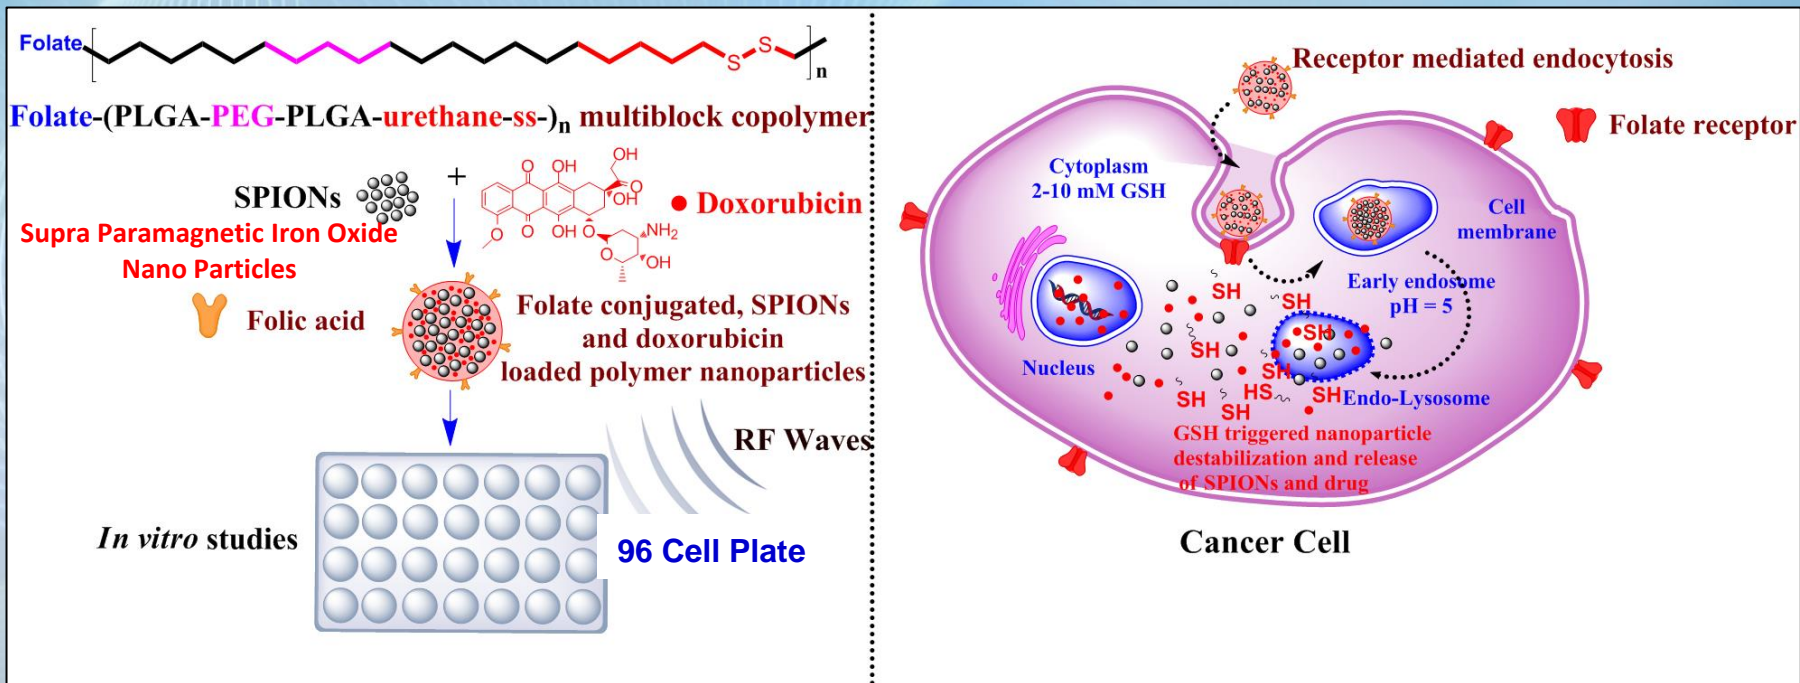


Source: C.Nehate, M. Alex, A. Kumar and Veena Koul, Material Science and Engineering C:Materials for Biological Applications, June 2017



RF Hyperthermia Treatment

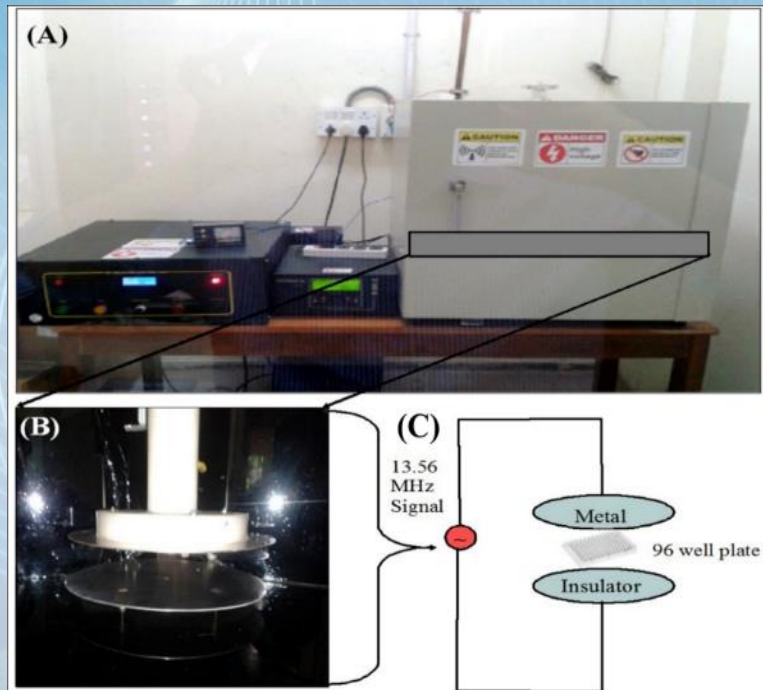


MDA-MB-231

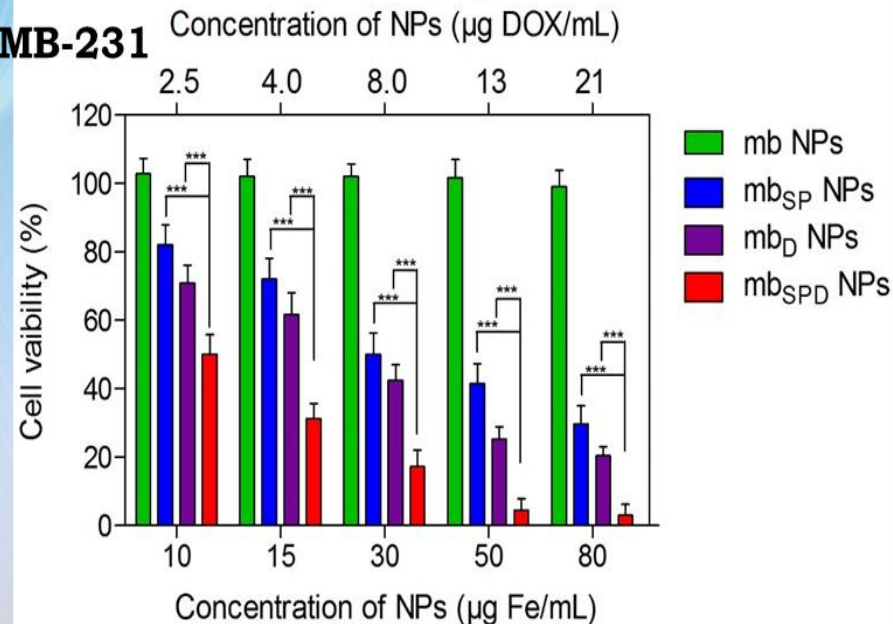

RF Exposure for 10 minutes at 50 Watts



Wearable Sensor Based System

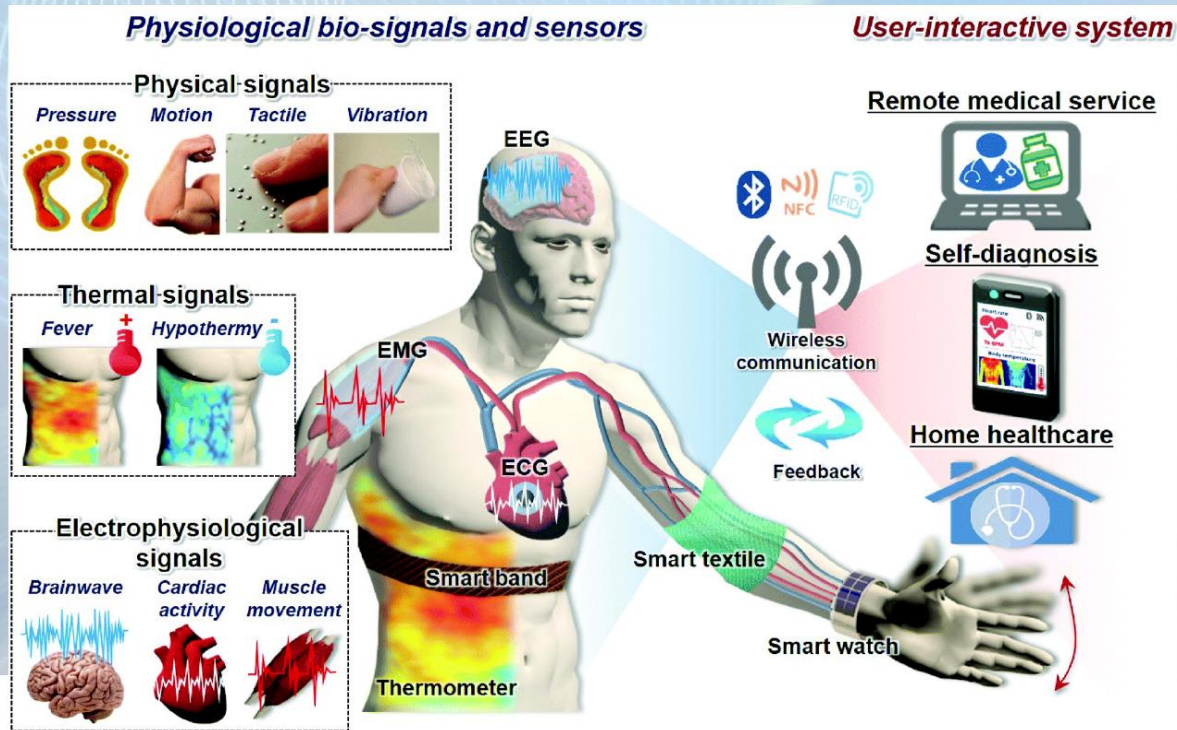




Through the Wall Radar for Detecting Vital Signs

IEEE SENSORS JOURNAL, VOL. 21, NO. 2, JANUARY 15, 2021



Through the Wall Human Subject Localization and Respiration Rate Detection Using Multichannel Doppler Radar

Harikesh^{ID}, *Student Member, IEEE*, Shakti Singh Chauhan, *Student Member, IEEE*, Ananjan Basu^{ID}, *Member, IEEE*, Mahesh P. Abegaonkar^{ID}, *Senior Member, IEEE*, and Shibani Kishen Koul^{ID}, *Life Fellow, IEEE*



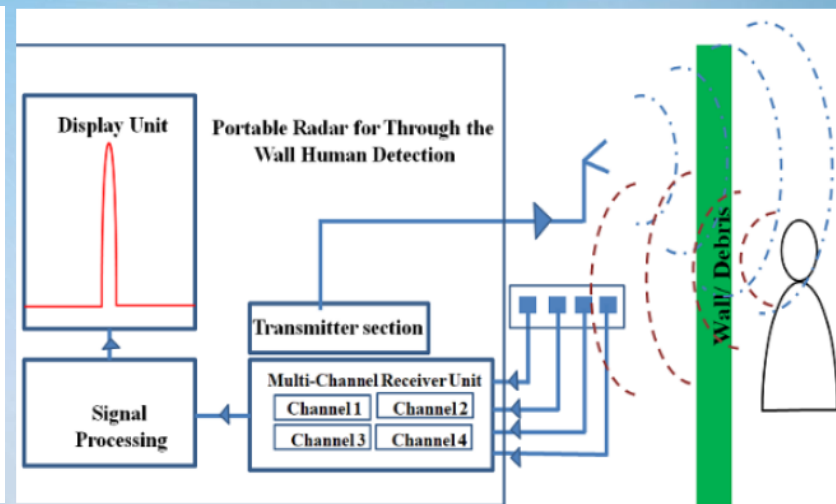


Sensors mounted on drone can be thrown at the location of building collapse to detect whether the buried humans are still alive. This will help in quick rescue operation and saving precious human lives

Source: IEEE Sensor Journal, January 2021




Recent Books (2021-2023)

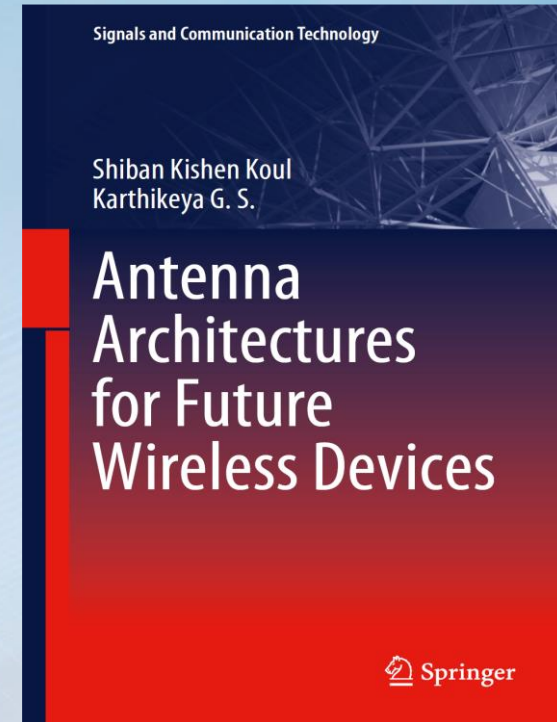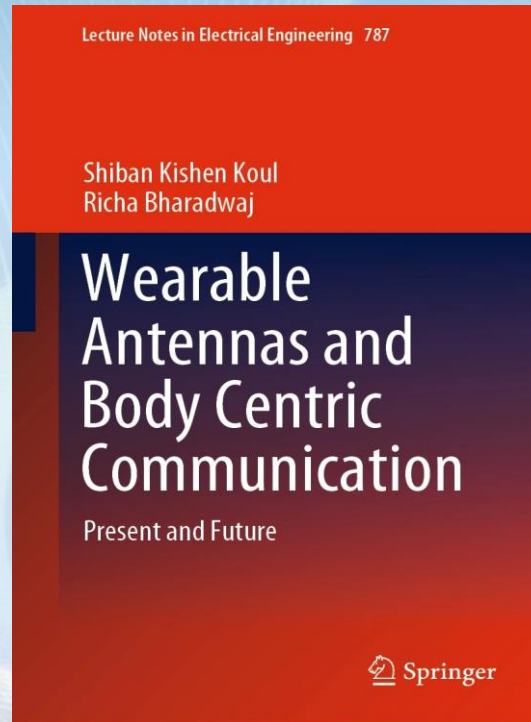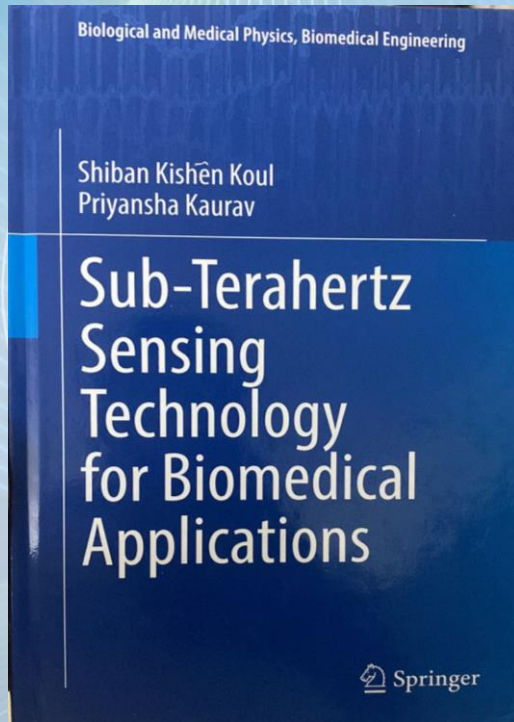

IEEE Computer Society 2023 Technical Predictions

**Remote
(Wireless)
and Wearable
Technologies
for Healthcare**

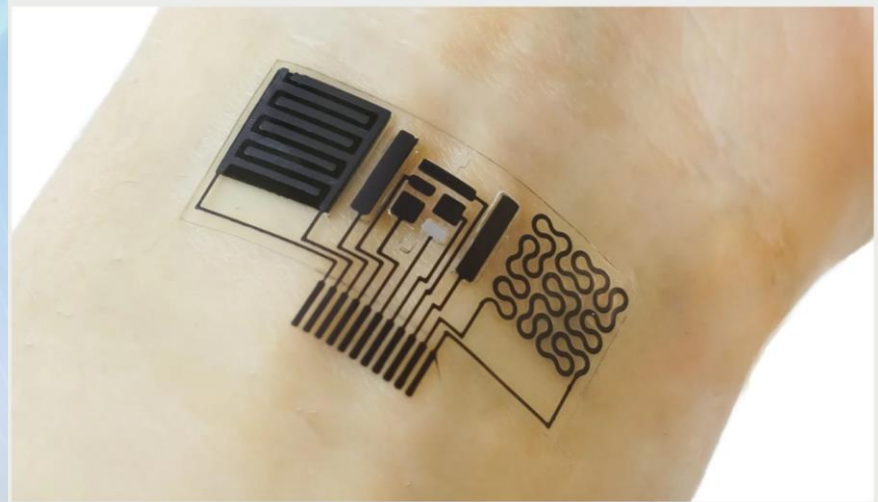

Caltech's team has experimented with different forms of energy to harvest for powering its e-skin, including human sweat and friction of materials during movement. WEI GAO/CALTECH

Source IEEE Spectrum 01 Nov.2023



Conclusions and Recommendations

NLCSSPR_9-12-2023

- **Whether we like it or not- Electromagnetic Waves are used everywhere.**
- **Need to join AP or MTT-S Society and learn MHz to THz Technologies.**
- **Require multiple skills such as knowledge of Basic Electromagnetics, Antenna Engineering, Microelectronics, Computer Science (AI,ML, Cloud Computing), Mechanical Engineering, Material Science and Bio-medical Engineering.**
- **Need to Collaborate with Medical doctors as well as Engineering Professions.**
- **Together we need to Serve Humanity**
- **Future will demand low-cost wearable and wireless devices**



**Thank
You for
Your
Kind
Attention**



Any Question ???